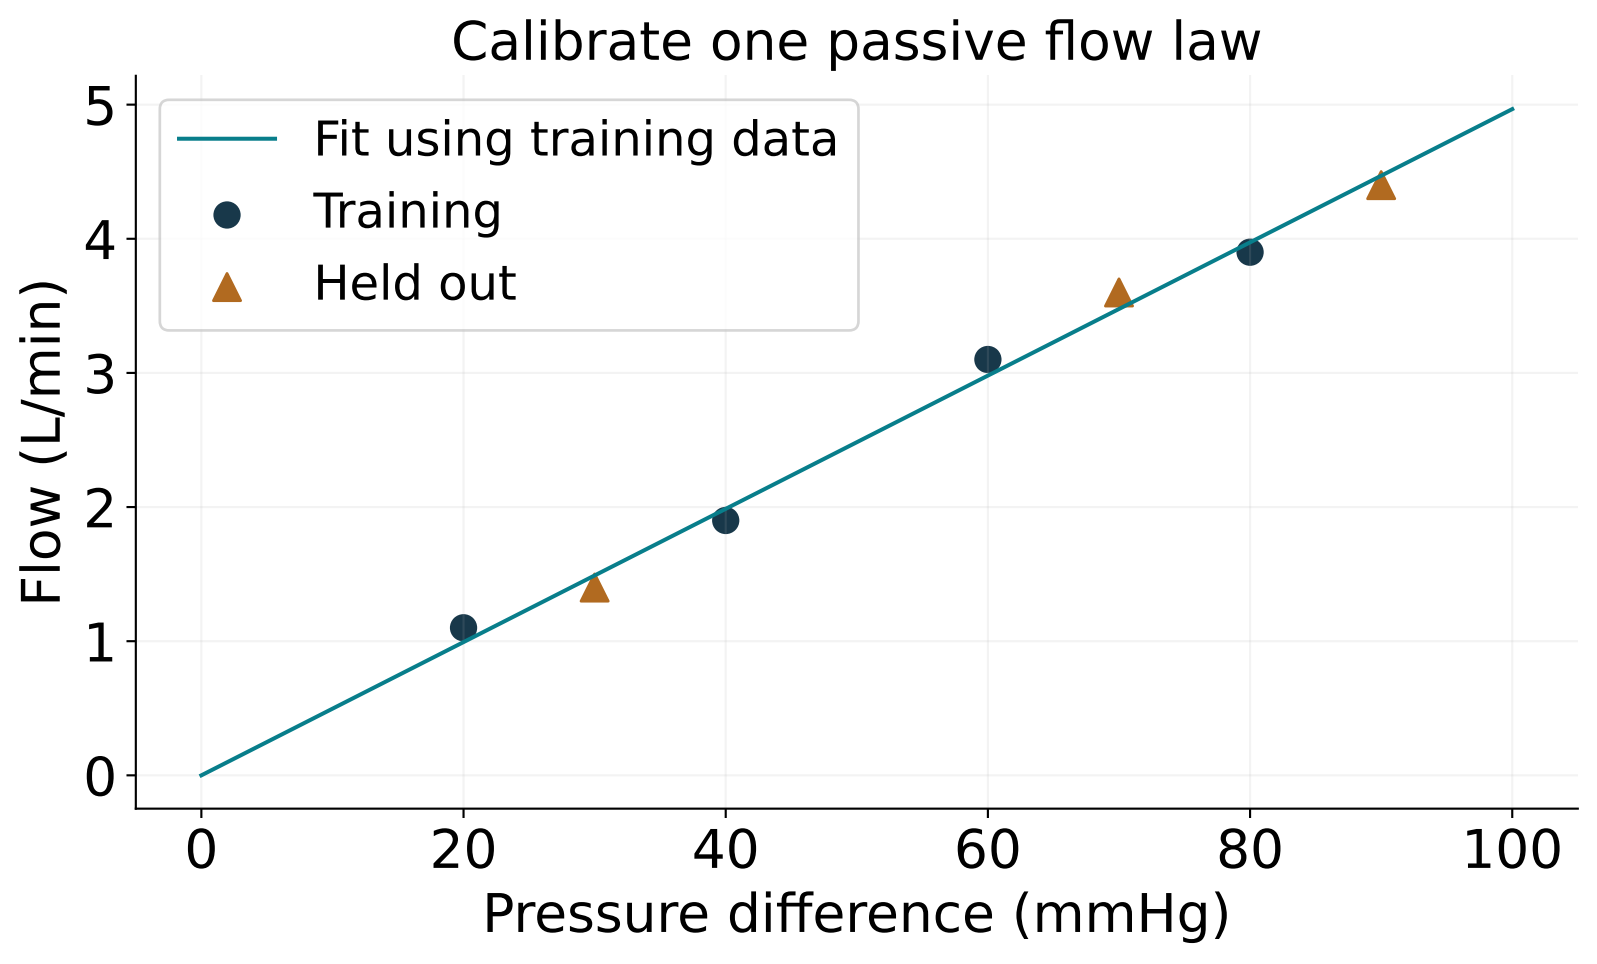

Calibrate one passive flow law
Fit using training data
Training
Held out
Flow (L/min)
Pressure difference (mmHg)
0
1
2
3
4
5
0
20
40
60
80
100