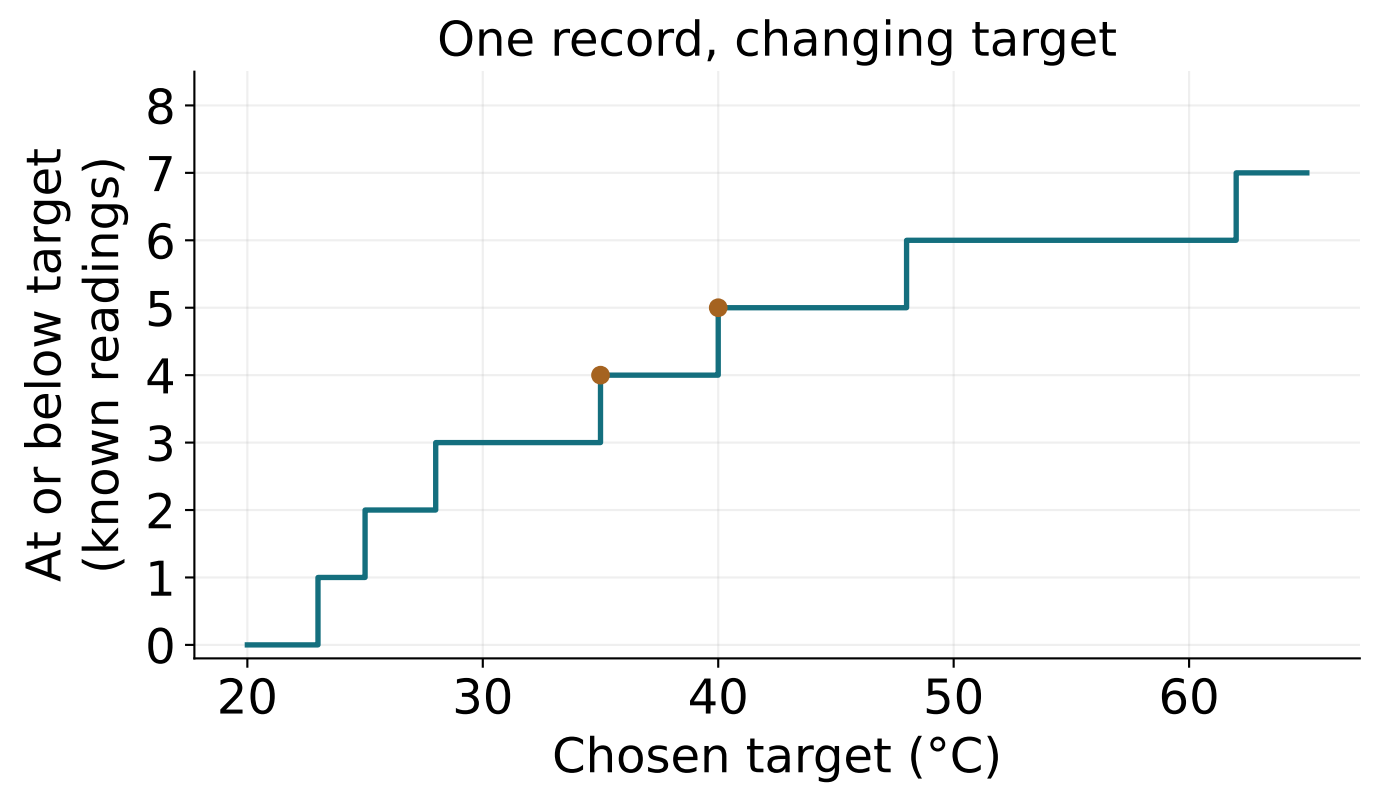

One record, changing target
At or below target
(known readings)
0
1
2
3
4
5
6
7
8
20
30
40
50
60
Chosen target (°C)